


Saliva testing is 36% more sensitive than the current gold standard.


This study determined that Naso-oro-pharyngeal (NOP) saliva specimens is less intrusive and provided more accurate and sensitive results for COVID-19 diagnosis than nasopharyngeal (NP) swabs and self-administered nasal swabs (SN). Lucence’s SAFER™ Saliva Collection Kit inactivates the SARS-CoV-2 virus in 45 seconds and keeps specimens viable at room temperature, making it safer and more convenient to use.

Teo AKJ, Choudhury Y, Tan IB, et al. Validation of Saliva and Self-Administered Nasal Swabs for COVID-19 Testing. medRxiv. 2020:2020.2008.2013.20173807.

01 Specimen Collection

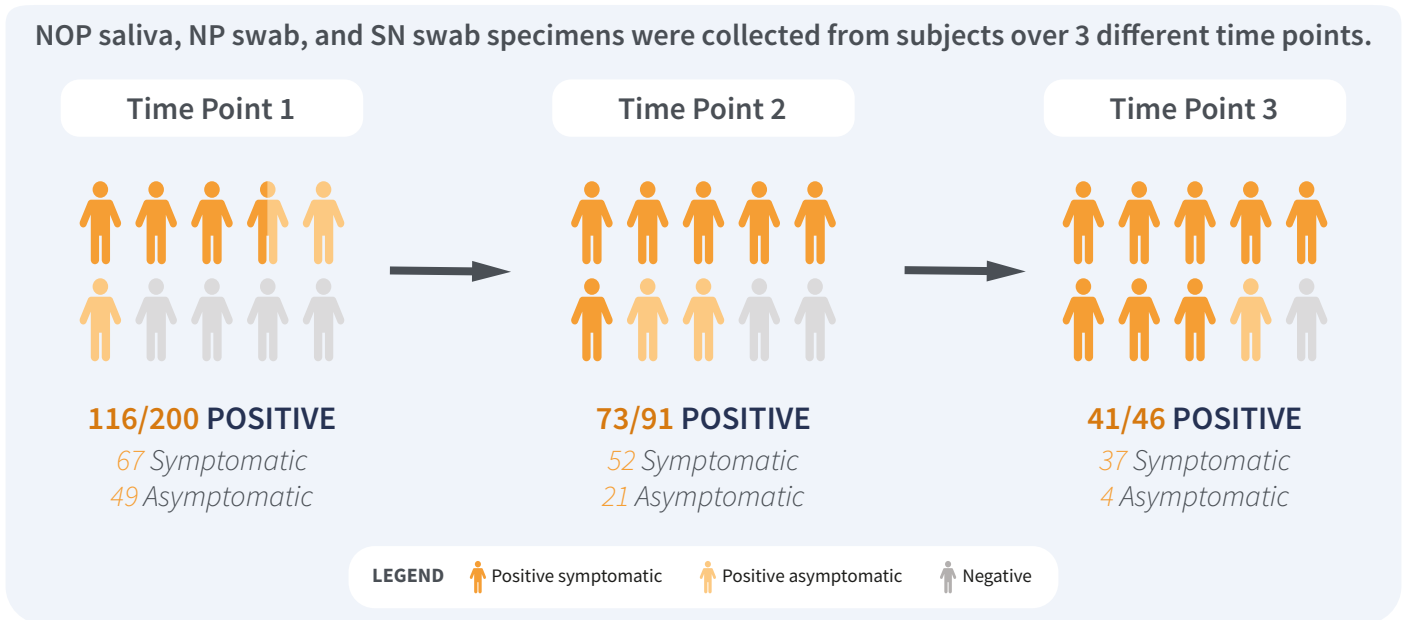

02 Results

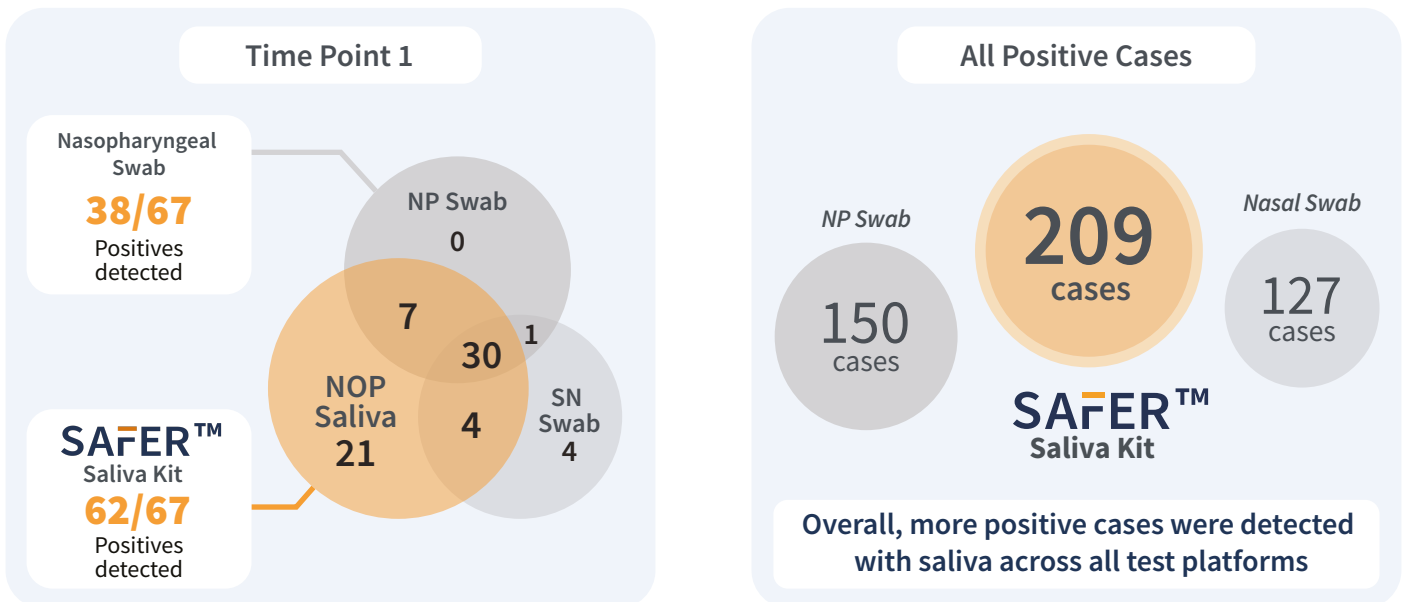

03 Conclusion

